

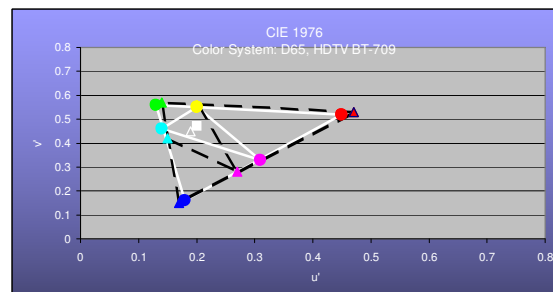
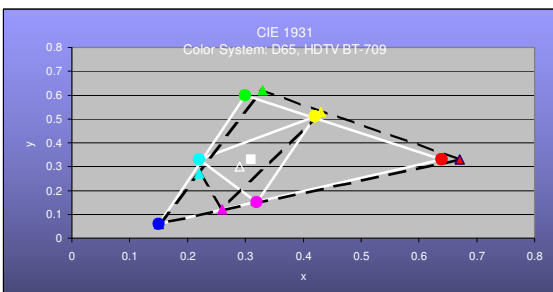
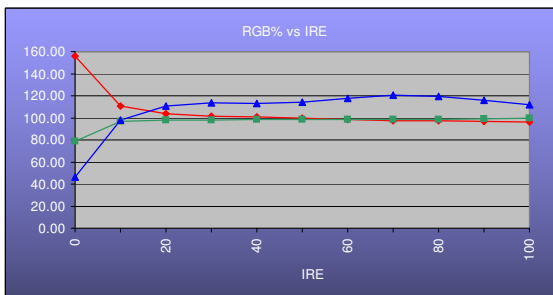
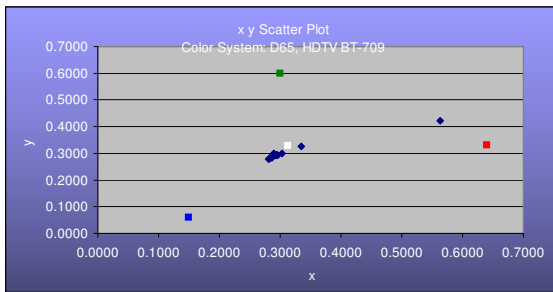
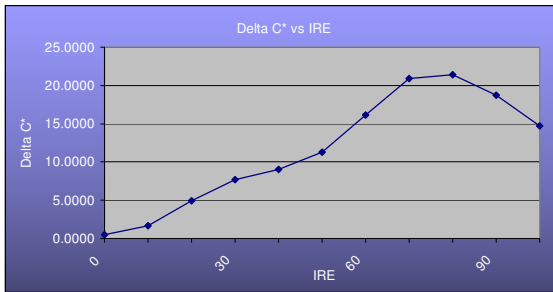


**Customer Name** Name withheld  
**Manufacturer** Hitachi  
**Model** 57wx20b  
**Serial Number**  
**Calibrated By** Summit HDTV  
**Calibration Date** March 18, 2010 (06:56:09 PM)  
**RGB Transform** RGB Transform : D65, HDTV BT-709  
**Luminance Units** fL

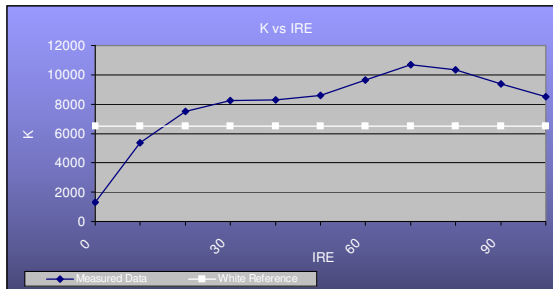

### Pre calibration

IRE	x	y	Y fl	Hz	Kelvin	Delta C*	R	R%	G	G%	B	B%	Measured Gamma	User Gamma
0	0.5630	0.4210	0.0230	0.00	1306	0.5100	1.5600	155.77	0.7860	78.68	0.4640	46.37	1.3500	0.0000
10	0.3350	0.3260	0.5190	0.00	5389	1.6390	1.1100	110.82	0.9660	96.67	0.9790	97.92	2.0900	0.5120
20	0.3030	0.2990	2.2130	0.00	7516	4.9490	1.0370	103.51	0.9770	97.74	1.1060	110.68	2.2000	2.3510
30	0.2960	0.2930	5.3960	0.00	8254	7.6690	1.0160	101.45	0.9800	98.05	1.1340	113.48	2.2300	5.7370
40	0.2950	0.2950	10.2390	0.00	8271	9.0280	1.0080	100.65	0.9830	98.35	1.1310	113.10	2.2700	10.8030
50	0.2930	0.2920	17.0090	0.00	8601	11.3210	0.9990	99.75	0.9840	98.49	1.1420	114.19	2.2800	17.6500
60	0.2860	0.2840	25.7590	0.00	9651	16.0980	0.9880	98.63	0.9830	98.37	1.1780	117.86	2.3300	26.3600
70	0.2810	0.2770	36.8680	0.00	10711	20.8780	0.9780	97.67	0.9820	98.28	1.2070	120.73	2.2300	37.0030
80	0.2820	0.2810	49.6840	0.00	10328	21.4190	0.9740	97.22	0.9850	98.58	1.1940	119.44	2.2200	49.6390
90	0.2860	0.2900	64.5560	0.00	9362	18.7100	0.9680	96.65	0.9920	99.20	1.1580	115.87	2.1700	64.3210
100	0.2900	0.3000	81.1000	0.00	8525	14.6800	0.9620	96.01	0.9980	99.87	1.1180	111.84		81.1000

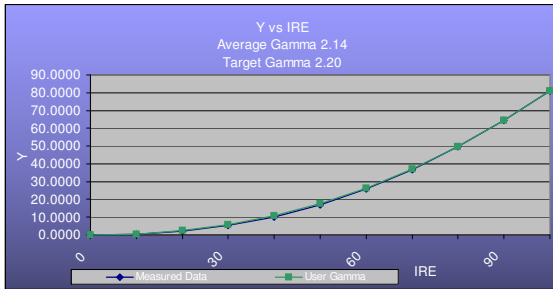

Customer Name Name withheld  
 Manufacturer Hitachi  
 Model 57xwx20b  
 Serial Number  
 Calibrated By Summit HDTV  
 Calibration Date March 18, 2010 (06:56:09 PM)  
 RGB Transform RGB Transform : D65, HDTV BT-709  
 Luminance Units fL



### Post Calibration

Customer Name Name withheld  
 Manufacturer Hitachi  
 Model 57xwx20b  
 Serial Number  
 Calibrated By Summit HDTV  
 Calibration Date March 18, 2010 (06:56:09 PM)  
 RGB Transform RGB Transform : D65, HDTV BT-709  
 Luminance Units fL



IRE	x	y	Y fL	Hz	Kelvin	DeltaC*	R	R%	G	G%	B	B%	Measured Gamma
0	0.3270	0.4180	0.0070	0.00	5332	0.0680	0.8530	85.19	1.0600	106.05	0.7240	72.43	1.3000
10	0.3020	0.3390	0.1410	0.00	7008	0.3620	0.9140	91.29	1.0250	102.57	0.9840	98.42	2.4300
20	0.3040	0.3260	0.7590	0.00	7016	0.7240	0.9660	96.42	1.0080	100.82	1.0210	102.17	2.3900
30	0.3050	0.3200	2.0010	0.00	7010	1.2890	0.9860	98.50	1.0000	100.07	1.0360	103.62	2.3800
40	0.3060	0.3190	3.9660	0.00	7024	1.9090	0.9920	99.08	0.9980	99.84	1.0410	104.15	2.3800
50	0.3070	0.3190	6.7380	0.00	6903	2.1180	1.0000	99.81	0.9960	99.68	1.0360	103.68	2.3500
60	0.3090	0.3220	10.3370	0.00	6761	1.8970	1.0030	100.18	0.9960	99.67	1.0270	102.74	2.3300
70	0.3110	0.3250	14.7970	0.00	6604	1.1870	1.0050	100.32	0.9970	99.78	1.0140	101.40	2.3000
80	0.3120	0.3260	20.1160	0.00	6570	1.0040	1.0040	100.28	0.9980	99.81	1.0100	101.04	2.2500
90	0.3110	0.3250	26.2130	0.00	6660	1.5410	1.0010	99.99	0.9980	99.83	1.0160	101.67	2.2900
100	0.3070	0.3200	33.3720	0.00	6893	3.3210	0.9980	99.60	0.9970	99.76	1.0340	103.45	

