

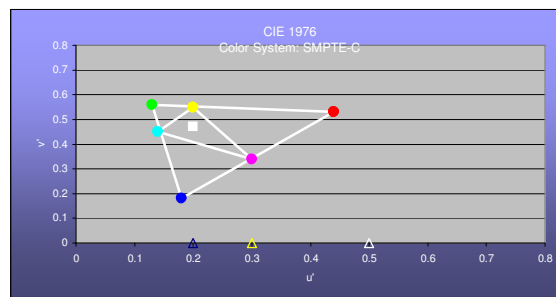
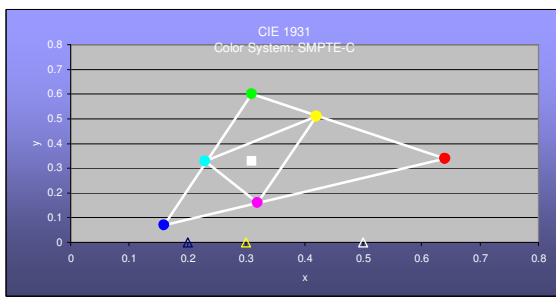
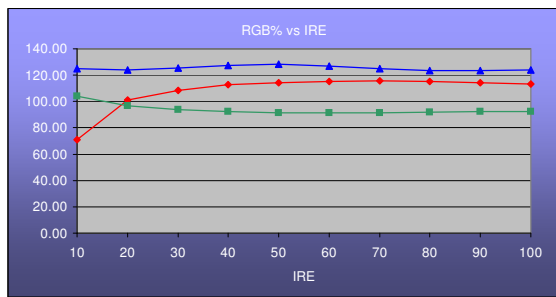
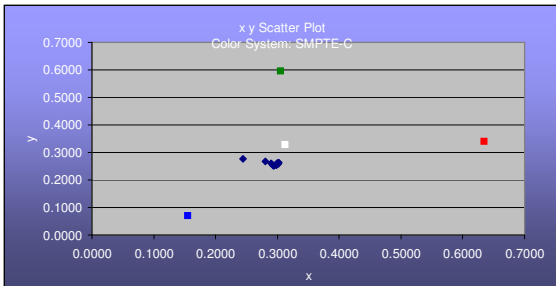
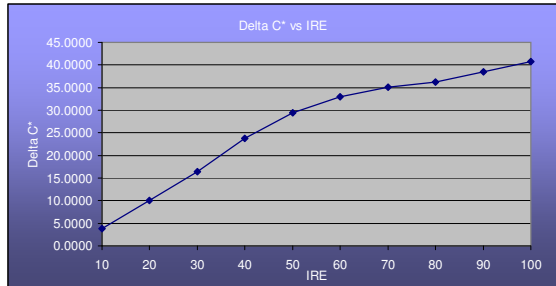


Customer Name Withheld
Manufacturer Mts
Model ws-55807
Serial Number
Calibrated By Summit HDTV
Calibration Date November 14, 2007 (06:16:20 PM)
RGB Transform : HDTV BT 709
Luminance Units fL

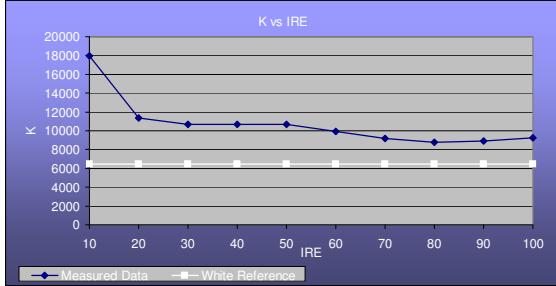

Pre Calibration All data Copyright SummitHDTV@2003-2009, www.SummitHDTV.com

IRE	x	y	Y fL	Hz	Kelvin	DeltaC*	R	R%	G	G%	B	B%	Measured Gamma	User Gamma
10	0.2440	0.2770	0.4070		17932	3.8860	0.7090	70.92	1.0400	103.96	1.2520	125.16	N/A	0.4770
20	0.2810	0.2680	2.2450		11350	10.0000	1.0120	101.23	0.9680	96.77	1.2390	123.84	2.3000	2.1920
30	0.2900	0.2610	5.7360		10707	16.4720	1.0860	108.56	0.9400	94.05	1.2560	125.55	2.5000	5.3490
40	0.2930	0.2540	11.6170		10673	23.8380	1.1270	112.73	0.9220	92.20	1.2750	127.46	2.2000	10.0720
50	0.2940	0.2520	18.8510		10709	29.4130	1.1430	114.31	0.9140	91.44	1.2830	128.30	2.2000	16.4550
60	0.2980	0.2540	28.3370		9904	32.9610	1.1520	115.18	0.9130	91.32	1.2690	126.88	2.0000	24.5750
70	0.3010	0.2580	38.5230		9150	35.0310	1.1570	115.68	0.9140	91.39	1.2510	125.08	2.1000	34.4970
80	0.3020	0.2620	50.8950		8774	36.2070	1.1500	115.03	0.9190	91.89	1.2350	123.51	1.9000	46.2770
90	0.3010	0.2620	63.7750		8910	38.5520	1.1430	114.35	0.9220	92.15	1.2360	123.57	1.6000	59.9650
100	0.2990	0.2610	75.6080		9276	40.7400	1.1330	113.36	0.9250	92.46	1.2420	124.16		75.6080

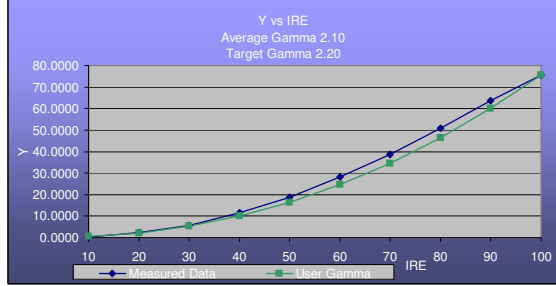

Customer Name Withheld
Manufacturer Mts
Model ws-55807
Serial Number
Calibrated By Summit HDTV
Calibration Date November 14, 2007 (06:16:20 PM)
RGB Transform RGB Transform : HDTV BT 709
Luminance Units fL
Post Calibration

Summit HDTV
 Your better image HDTV calibration resource
www.SummitHDTV.com



IRE	x	y	Y fL	Hz	Kelvin	DeltaC*	R	R%	G	G%	B	B%	Measured Gamma	User Gamma
10	0.2970	0.3020	0.1030	60.00	7944	0.3660	0.9930	99.33	0.9910	99.06	1.1050	110.48	N/A	0.0870
20	0.3080	0.3160	0.4070	60.00	6897	0.7300	1.0140	101.41	0.9910	99.08	1.0470	104.68	2.1000	0.4010
30	0.3130	0.3210	0.9500	60.00	6565	1.0320	1.0220	102.16	0.9910	99.10	1.0240	102.36	2.3000	0.9800
40	0.3140	0.3250	1.8600	60.00	6470	0.8140	1.0160	101.62	0.9940	99.41	1.0100	101.00	2.1000	1.8450
50	0.3140	0.3260	3.0040	60.00	6436	0.9100	1.0150	101.55	0.9950	99.47	1.0060	100.63	2.3000	3.0140
60	0.3150	0.3270	4.5780	60.00	6392	0.8520	1.0180	101.78	0.9940	99.43	1.0040	100.35	2.2000	4.5010
70	0.3130	0.3270	6.3800	60.00	6486	0.4580	1.0070	100.76	0.9970	99.73	1.0050	100.46	2.3000	6.3180
80	0.3140	0.3300	8.6280	60.00	6425	0.3640	1.0030	100.31	1.0000	99.96	0.9950	99.48	2.1000	8.4760
90	0.3110	0.3280	11.0310	60.00	6609	0.4230	0.9940	99.44	1.0010	100.11	1.0060	100.61	2.2000	10.9830
100	0.3110	0.3260	13.8480	60.00	6636	0.8580	0.9990	99.89	0.9990	99.91	1.0120	101.23		13.8480

